




## Differentiated Thyroid Carcinoma

### Algorithm for the follow-up after initial treatment (surgery and radioiodine ablation)\*

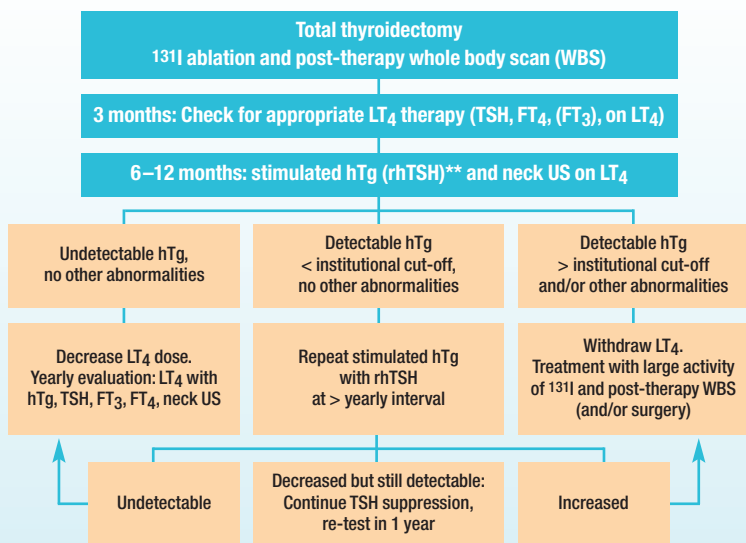


### Thermo Scientific™ B·R·A·H·M·S™ Thyroglobulin Assays

- B·R·A·H·M·S **Tg-pluS** RIA/LIA
- B·R·A·H·M·S **Tg-S** RIA/Recovery RIA
- B·R·A·H·M·S **hTg** KRYPTOR (with Recovery)
- B·R·A·H·M·S **hTg sensitive** KRYPTOR (with Recovery)

\* Adapted from: Pacini F et al. Eur J Endocrinol. 2006;154(6):787-803, Page 797, Fig. 2

\*\* If basal hTg is detectable there is no need for rhTSH stimulation and the patient needs imaging and/or therapy.

## Algorithm for follow-up in TgAb positive patients\*

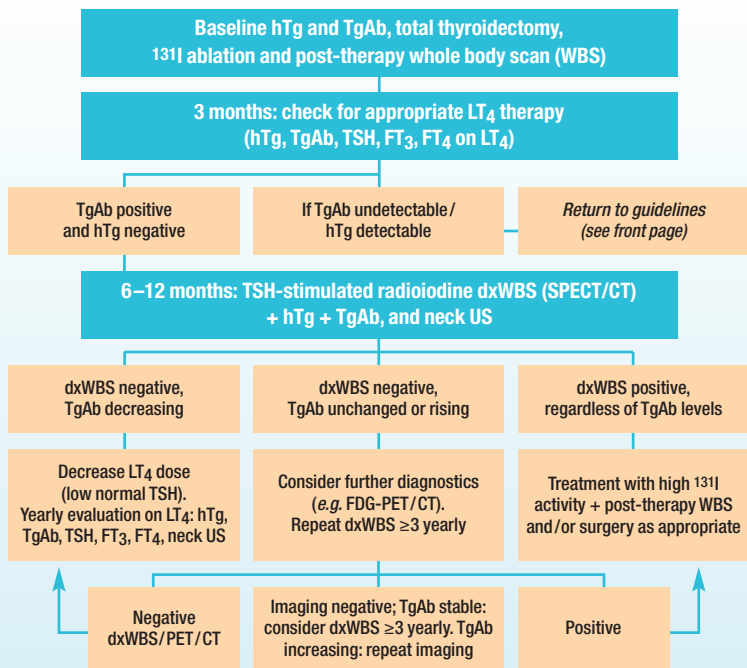

\* Adapted from: Verburg FA et al. Eur Thyroid J Vol. 1, Suppl. 1,2012; P260

## Thermo Scientific™ B-R-A-H-M-S™ Thyroglobulin Autoantibody Assays

- B-R-A-H-M-S anti-Tg<sub>n</sub> KRYPTOR/RIA/LIA

© 2012 Thermo Fisher Scientific Inc. All rights reserved. KRYPTOR is a registered trademark of CIS bio international, licensed for use by B-R-A-H-M-S, a part of Thermo Fisher Scientific. All other trademarks are the property of Thermo Fisher Scientific Inc. and its subsidiaries. All data regarding specifications, terms and pricing correspond to the existing knowledge at the time of the printing. We are not responsible for any errors, misprints or changes. Reprint, also in parts, solely with prior written consent of B-R-A-H-M-S GmbH.

Thermo Fisher Scientific products are distributed worldwide; not all intended uses and applications mentioned in this printing are registered in every country.

### Clinical Diagnostics

Thermo Fisher Scientific  
B-R-A-H-M-S GmbH  
Neuendorfstr. 25  
16761 Hennigsdorf  
Germany

+49-(0)3302-883-0  
+49-(0)3302-883-100 fax  
info.brahms@thermofisher.com

www.thermoscientific.com/brahms

**Thermo**  
SCIENTIFIC  
Part of Thermo Fisher Scientific